

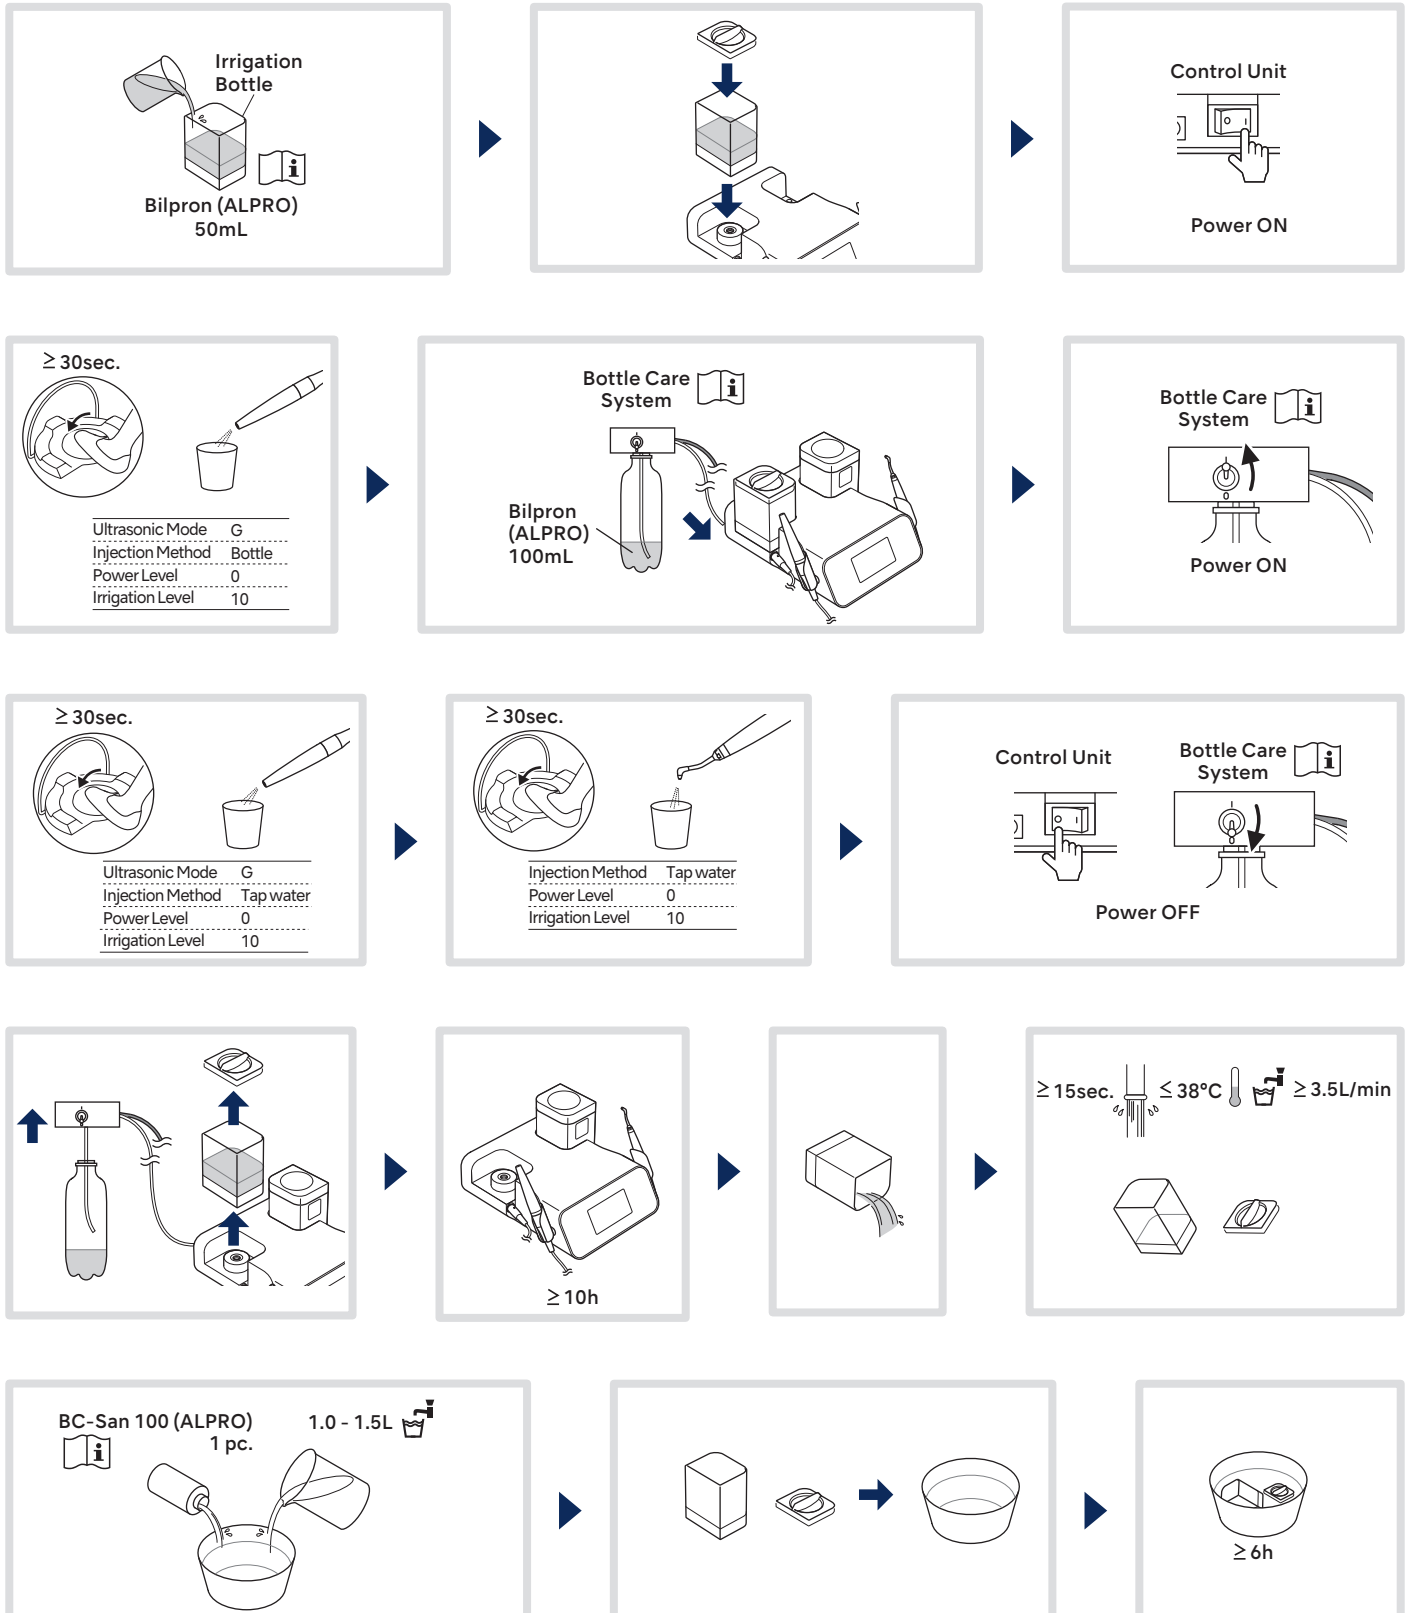
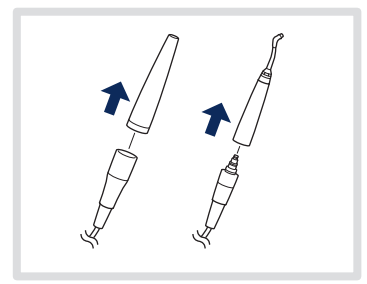
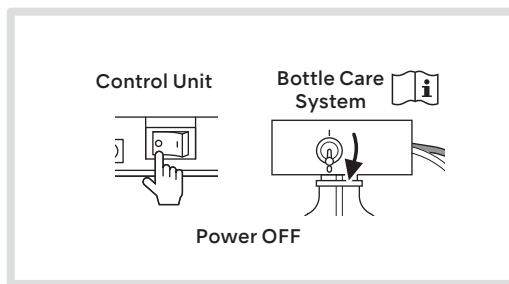
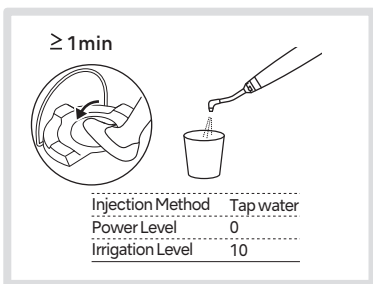
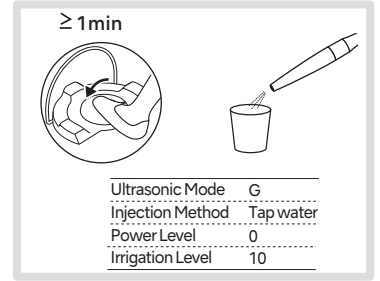

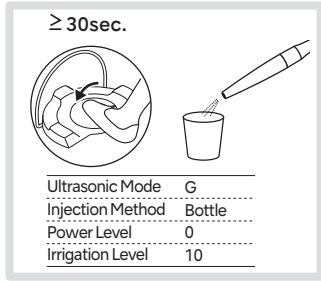


- ⚠ Perform cleaning and disinfection of the ultrasonic handpiece and powder handpiece before reprocessing the water circuit.
- Disinfection with ALPRO Bilpron (undiluted) is recommended as maintenance twice a week and before the weekend or periods of closure/inactivity.



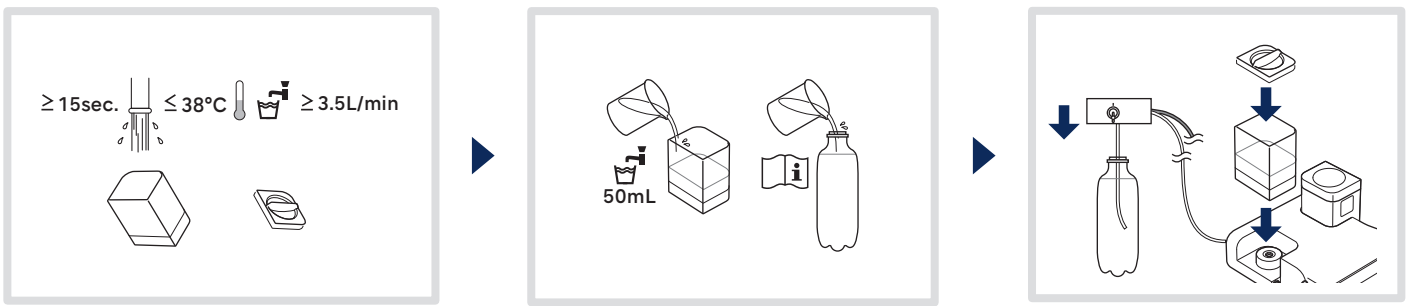

2 Packaging, Sterilizing and Drying

Type	Class N	Class B
Temperature	132°C	134°C
Full Cycle Time	≥15min	3-18min
Drying Time	≥30min	≥30min

Use a sterilization pouch that conforms to ISO 11607-1. Seal the pouch. Maximum temperature for NSK instruments is 135°C.

Perform steam sterilization using the conditions above. Use a steam sterilizer to perform sterilization.

CAUTION

✓ Steam sterilization
✗ Plasma
✗ EO

3 Storage

